

# User Manual

**Catalog No. EKE60396**

## **Human MMRN1 (Multimerin 1) ELISA Kit**

Version 20180310

The manual may be updated as a result of continuous improvements.  
Please refer to the hard copy manual included in the kit for your experiment.

**This kit is for scientific research use only. Not for use in diagnostic procedures.**

### **Intended use**

This ELISA kit applies to the in vitro quantitative determination of Human MMRN1 concentrations in serum, plasma and other biological fluids.

### **Specification**

- Sensitivity: 46.88 pg/mL
- Detection Range: 78.13-5000 pg/mL
- Specificity: This kit recognizes Human MMRN1 in samples. No significant cross-reactivity or interference between Human MMRN1 and analogues was observed.
- Repeatability: Coefficient of variation is < 10%.

## Test principle

This ELISA kit uses the Sandwich-ELISA principle. The micro ELISA plate provided in this kit has been pre-coated with an antibody specific to Human MMRN1. Standards or samples are added to the micro ELISA plate wells and combined with the specific antibody. Then a biotinylated detection antibody specific for Human MMRN1 and Avidin-Horseradish Peroxidase (HRP) conjugate are added successively to each micro plate well and incubated. Free components are washed away. The substrate solution is added to each well. Only those wells that contain Human MMRN1, biotinylated detection antibody and Avidin-HRP conjugate will appear blue in color. The enzyme-substrate reaction is terminated by the addition of stop solution and the color turns yellow. The optical density (OD) is measured spectrophotometrically at a wavelength of  $450\text{ nm} \pm 2\text{ nm}$ . The OD value is proportional to the concentration of Human MMRN1. You can calculate the concentration of Human MMRN1 in the samples by comparing the OD of the samples to the standard curve.

## Kit components & Storage

An unopened kit can be stored at 4°C for 1 month. If the kit is not to be used within 1 month, store the items separately according to the following conditions once the kit is received.

| Item                                          | Specifications     | Storage                              |
|-----------------------------------------------|--------------------|--------------------------------------|
| Micro ELISA Plate (Dismountable)              | 8 wells ×12 strips | -20°C, 6 months                      |
| Reference Standard                            | 2 vials            |                                      |
| Concentrated Biotinylated Detection Ab (100×) | 1 vial, 120 µL     |                                      |
| Concentrated HRP Conjugate (100×)             | 1 vial, 120 µL     | -20°C (protect from light), 6 months |
| Reference Standard & Sample Diluent           | 1 vial, 20 mL      | 4°C, 6 months                        |
| Biotinylated Detection Ab Diluent             | 1 vial, 14 mL      |                                      |
| HRP Conjugate Diluent                         | 1 vial, 14 mL      |                                      |
| Concentrated Wash Buffer (25×)                | 1 vial, 30 mL      |                                      |
| Substrate Reagent                             | 1 vial, 10 mL      | 4°C (protect from light)             |
| Stop Solution                                 | 1 vial, 10 mL      | 4°C                                  |
| Plate Sealer                                  | 5 pieces           |                                      |
| Product Description                           | 1 copy             |                                      |
| Certificate of Analysis                       | 1 copy             |                                      |

Note: All reagent bottle caps must be tightened to prevent evaporation and microbial pollution.

The volume of reagents in partial shipments is a little more than the volume marked on the label, please use accurate measuring equipment instead of directly pouring into the vial(s).

## Other supplies required

Microplate reader with 450 nm wavelength filter

High-precision transfer pipette, EP tubes and disposable pipette tips

Incubator capable of maintaining 37°C

Deionized or distilled water  
Absorbent paper  
Loading slot for Wash Buffer

#### **Note**

1. Please wear lab coats, eye protection and latex gloves for protection. Please perform the experiment following the national security protocols of biological laboratories, especially when analyzing blood samples or other bodily fluids.
2. A freshly opened ELISA Plate may appear to have a water-like substance, which is normal and will not have any impact on the experimental results.
3. Do not reuse the diluted standard, biotinylated detection Ab working solution, concentrated HRP conjugate working solution. The unspent, undiluted concentrated biotinylated detection Ab (100×) and other stock solutions should be stored according to the storage conditions in the above table.
4. The microplate reader should have a 450 ( $\pm 10$  nm) filter installed and a detector that can detect the wavelength. The optical density should be within 0~3.5.
5. Do not mix or use components from other lots.
6. Change pipette tips in between adding standards, in between sample additions, and in between reagent additions. Also, use separate reservoirs for each reagent.

#### **Sample collection**

**Serum:** Allow samples to clot for 2 hours at room temperature or overnight at 4°C before centrifugation for 15 min at 1000×g at 2~8°C. Collect the supernatant to carry out the assay. Blood collection tubes should be disposable, and be non-endotoxin.

**Plasma:** Collect plasma using EDTA or heparin as an anticoagulant. Centrifuge samples for 15 min at 1000×g at 2~8°C within 30 min of collection. Collect the supernatant to carry out the assay. Hemolyzed samples are not suitable for ELISA assay!

**Cell lysates:** For adherent cells, gently wash the cells with a moderate amount of pre-cooled PBS and dissociate the cells using trypsin. Collect the cell suspension into a centrifuge tube and centrifuge for 5 min at 1000×g. Discard the medium and wash the cells 3 times with pre-cooled PBS. For each  $1 \times 10^6$  cells, add 150-250  $\mu$ L of pre-cooled PBS to keep the cells suspended. Repeat the freeze-thaw process several times until the cells are fully lysed. Centrifuge for 10 min at 1500×g at 4°C. Remove the cell fragments, collect the supernatant to carry out the assay. Avoid repeated freeze-thaw cycles.

**Tissue homogenates:** It is recommended to get detailed references from the literature before analyzing different tissue types. For general information, hemolyzed blood may affect the results, so the tissues should be minced into small pieces and rinsed in ice-cold PBS (0.01 M, pH=7.4) to remove excess blood thoroughly. Tissue pieces

should be weighed and then homogenized in PBS (tissue weight (g): PBS (mL) volume=1:9) with a glass homogenizer on ice. To further break down the cells, you can sonicate the suspension with an ultrasonic cell disrupter or subject it to freeze-thaw cycles. The homogenates are then centrifuged for 5 min at 5000×g to get the supernatant.

**Cell culture supernatant or other biological fluids:** Centrifuge samples for 20 min at 1000×g at 2~8°C. Collect the supernatant to carry out the assay.

**Note for sample:**


1. Samples should be assayed within 7 days when stored at 4°C, otherwise samples must be divided up and stored at -20°C (≤1 month) or -80°C (≤3 months). Avoid repeated freeze-thaw cycles.
2. Please predict the concentration before assaying. If the sample concentration is not within the range of the standard curve, users must determine the optimal sample dilutions for their particular experiments.
3. If the sample type is not included in the manual, a preliminary experiment is suggested to verify the validity.
4. If a lysis buffer is used to prepare tissue homogenates or cell culture supernatant there is a possibility of causing a deviation, due to the introduced chemical substance.
5. Some recombinant protein may not be detected due to a mismatching with the coated antibody or detection antibody.

**Reagent preparation**

Bring all reagents to room temperature (18~25°C) before use. Follow the Microplate reader manual for set-up before OD measurement.

1. **Wash Buffer:** Dilute 30 mL of Concentrated Wash Buffer with 720mL of deionized or distilled water to prepare 750 mL of Wash Buffer. Note: if crystals have formed in the concentrate, warm it in a 40°C water bath and mix it gently until the crystals have completely dissolved.
2. **Standard working solution:** Centrifuge the standard at 10,000×g for 1 min. Add 1.0 mL of Reference Standard & Sample Diluent, let it stand for 10 min and invert it gently several times. After it dissolves fully, mix it thoroughly with a pipette tip. This reconstitution produces a working solution of 5000 pg/mL. Then make serial dilutions as needed. The recommended dilution gradient is as follows: 5000, 2500, 1250, 625, 312.5, 156.25, 78.13, 0 pg/mL.

Dilution method: Take 7 EP tubes, add 500μL of Reference Standard & Sample Diluent to each tube. Pipette 500 μL of the 5000 pg/mL working solution to the first tube and mix up to produce a 2500 pg/mL working solution. Pipette 500 μL of the solution from the former tube into the latter one according to these steps. The illustration below is for reference. Note: the last tube is regarded as a blank. Don't pipette solution into it from the former tube.

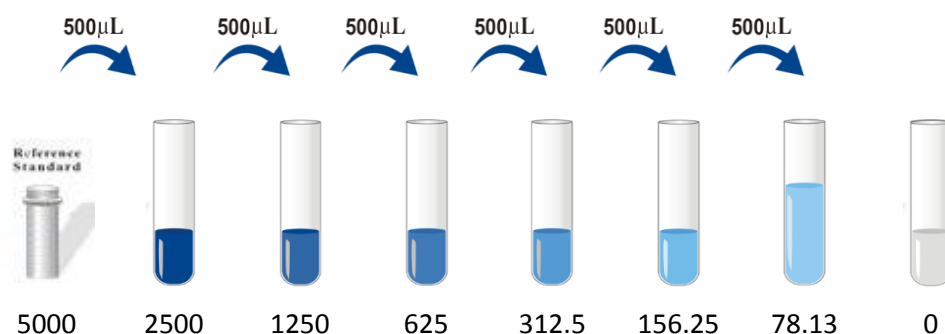

1. **Biotinylated Detection Ab working solution:** Calculate the required amount before the experiment (100 µL/well). In preparation, slightly more than calculated should be prepared. Centrifuge the stock tube before use, dilute the 100× Concentrated Biotinylated Detection Ab to a 1×working solution with Biotinylated Detection Ab Diluent.
2. **Concentrated HRP Conjugate working solution:** Calculate the required amount before the experiment (100 µL/well). In preparation, slightly more than calculated should be prepared. Dilute the 100× Concentrated HRP Conjugate to a 1× working solution with Concentrated HRP Conjugate Diluent.

#### Assay procedure

1. Add the **Standard working solution** to the first two columns: Each concentration of the solution is added in duplicate, to one well each, side by side (100 µL for each well). Add the samples to the other wells (100 µL for each well). Cover the plate with the sealer provided in the kit. Incubate for 90 min at 37°C. Note: solutions should be added to the bottom of the micro ELISA plate well, avoid touching the inside wall and causing foaming as much as possible.
2. Remove the liquid out of each well, do not wash. Immediately add 100 µL of **Biotinylated Detection Ab working solution** to each well. Cover with the Plate sealer. Gently mix. Incubate for 1 hour at 37°C.
3. Aspirate or decant the solution from each well, add 350 µL of **Wash Buffer** to each well. Soak for 1~2 min and aspirate or decant the solution from each well and pat it dry against clean absorbent paper. Repeat this wash step 3 times. Note: a microplate washer can be used in this and other wash steps.
4. Add 100 µL of **HRP Conjugate working solution** to each well. Cover with the Plate sealer. Incubate for 30 min at 37°C.
5. Aspirate or decant the solution from each well, repeat the wash process five times as conducted in step 3.
6. Add 90 µL of **Substrate Reagent** to each well. Cover with a new plate sealer. Incubate for about 15 min at 37°C. Protect the plate from light. Note: the reaction time can be shortened or extended according to the actual color change, but no more than 30 min.
7. Add 50 µL of **Stop Solution** to each well. Note: Adding the stop solution should be done in the same order as the substrate solution.
8. Determine the optical density (OD value) of each well at once with a micro-plate reader set to 450 nm.

#### Calculation of results

Average the duplicate readings for each standard and sample, then subtract the average zero standard optical


density reading. Plot a four-parameter logistic curve on log-log graph paper, with standard concentration on the x-axis and OD values on the y-axis.

If the samples have been diluted, the concentration calculated from the standard curve must be multiplied by the dilution factor. If the OD of the sample surpasses the upper limit of the standard curve, you should re-test it with an appropriate dilution. The actual concentration is the calculated concentration multiplied by the dilution factors including the amounts used in the sample preparation procedure.

### Typical data

As the OD values of the standard curve may vary according to the conditions of the actual assay performance (e.g. operator, pipetting technique, washing technique or temperature effects), the operator should establish a standard curve for each test. Typical standard curve data is provided below for reference only.

|                       |       |       |       |       |       |                   |       |       |
|-----------------------|-------|-------|-------|-------|-------|-------------------|-------|-------|
| Concentration (pg/mL) | 5000  | 2500  | 1250  | 625   | 312.5 | $\frac{156.2}{5}$ | 78.13 | 0     |
| OD                    | 2.543 | 1.716 | 0.983 | 0.459 | 0.248 | 0.173             | 0.119 | 0.064 |
| Corrected OD          | 2.479 | 1.652 | 0.919 | 0.395 | 0.184 | 0.109             | 0.055 | -     |

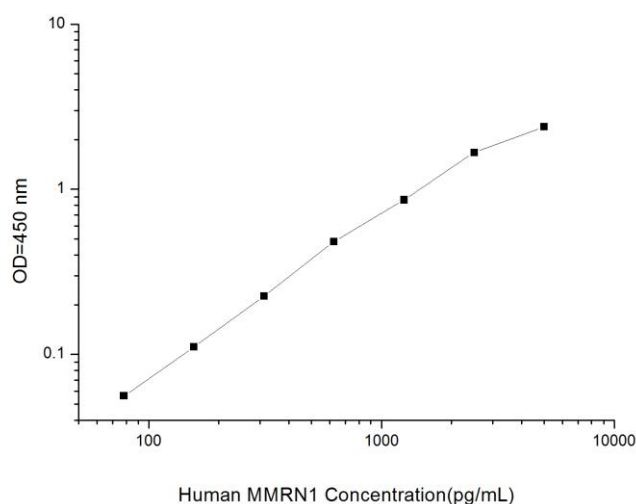

**Precision**

Intra-assay Precision (Precision within an assay): 3 samples with low, mid range and high level Human MMRN1 were tested 20 times on one plate, respectively.

Inter-assay Precision (Precision between assays): 3 samples with low, mid range and high level Human MMRN1 were tested on 3 different plates, 20 replicates in each plate.

|                    | Intra-assay Precision |        |         | Inter-assay Precision |        |         |
|--------------------|-----------------------|--------|---------|-----------------------|--------|---------|
| Sample             | 1                     | 2      | 3       | 1                     | 2      | 3       |
| n                  | 20                    | 20     | 20      | 20                    | 20     | 20      |
| Mean (pg/mL)       | 236.70                | 545.51 | 1682.79 | 222.73                | 492.13 | 1789.76 |
| Standard deviation | 16.31                 | 31.31  | 83.30   | 11.96                 | 22.83  | 69.98   |
| CV (%)             | 6.89                  | 5.74   | 4.95    | 5.37                  | 4.64   | 3.91    |

**Recovery**

The recovery of Human MMRN1 spiked at three different levels in samples throughout the range of the assay was evaluated in various matrices.

| Sample Type              | Range (%) | Average Recovery (%) |
|--------------------------|-----------|----------------------|
| Serum (n=5)              | 85-96     | 91                   |
| EDTA plasma (n=5)        | 94-109    | 100                  |
| Cell culture media (n=5) | 89-101    | 96                   |

**Linearity**

Samples were spiked with high concentrations of Human MMRN1 and diluted with Reference Standard & Sample Diluent to produce samples with values within the range of the assay.

|      |             | Serum (n=5) | EDTA plasma (n=5) | Cell culture media (n=5) |
|------|-------------|-------------|-------------------|--------------------------|
| 1:2  | Range (%)   | 94-106      | 92-108            | 94-105                   |
|      | Average (%) | 101         | 99                | 100                      |
| 1:4  | Range (%)   | 94-105      | 86-97             | 81-95                    |
|      | Average (%) | 100         | 92                | 88                       |
| 1:8  | Range (%)   | 93-108      | 82-93             | 81-96                    |
|      | Average (%) | 100         | 87                | 88                       |
| 1:16 | Range (%)   | 90-103      | 82-97             | 82-94                    |
|      | Average (%) | 96          | 89                | 88                       |

## Troubleshooting

| Problem                  | Causes                                      | Solutions                                                                                          |
|--------------------------|---------------------------------------------|----------------------------------------------------------------------------------------------------|
| Poor standard curve      | Inaccurate pipetting                        | Check pipettes.                                                                                    |
|                          | Improper standard dilution                  | Ensure you briefly spin the vial of standard and dissolve the powder thoroughly by gentle mixing.  |
|                          | Wells are not completely aspirated          | Completely aspirate wells in between steps.                                                        |
| Low signal               | Insufficient incubation time                | Ensure sufficient incubation time.                                                                 |
|                          | Incorrect assay temperature                 | Use recommended incubation temperature. Bring substrate to room temperature before use.            |
|                          | Inadequate reagent volumes                  | Check pipettes and ensure correct preparation.                                                     |
|                          | Improper dilution                           |                                                                                                    |
|                          | HRP conjugate inactive or TMB failure       | Mix HRP conjugate and TMB, rapid coloring.                                                         |
| Deep color but low value | Plate reader setting is not optimal         | Verify the wavelength and filter setting on the Microplate reader.                                 |
|                          |                                             | Turn on the Microplate Reader ahead to pre-heat.                                                   |
| Large CV                 | Inaccurate pipetting                        | Check pipettes.                                                                                    |
| High background          | Concentration of target protein is too high | Use recommended dilution factor.                                                                   |
|                          | Plate is insufficiently washed              | Review the manual for proper wash. If using a plate washer, check that all ports are unobstructed. |
|                          | Contaminated wash buffer                    | Prepare fresh wash buffer.                                                                         |
| Low sensitivity          | Improper storage of the ELISA kit           | All the reagents should be stored according to the instructions.                                   |
|                          | Stop solution is not added                  | Stop solution should be added to each well before measurement.                                     |



## SUMMARY

1. Add 100  $\mu$ L standard or sample to each well. Incubate for 90 min at 37°C .
2. Remove the liquid. Add 100  $\mu$ L Biotinylated Detection Ab. Incubate for 1 hour at 37°C.
3. Aspirate and wash 3 times.
4. Add 100  $\mu$ L HRP Conjugate. Incubate for 30 min at 37°C.
5. Aspirate and wash 5 times.
6. Add 90  $\mu$ L Substrate Reagent. Incubate for 15 min at 37°C.
7. Add 50  $\mu$ L Stop Solution. Read at 450 nm immediately.
8. Calculation of results.

## Declaration

1. Limited by current conditions and scientific technology, we can't conduct comprehensive identification and analysis on all the raw material provided. So there might be some qualitative and technical risks for users using the kit.
2. The final experimental results will be closely related to the validity of products, operational skills of the operators and the experimental environment. Please make sure that sufficient samples are available.
3. To get the best results, please only use the reagents supplied by the manufacturer and strictly comply with the instructions!
4. Incorrect results may occur because of incorrect operations during the reagent preparation and loading, as well as incorrect parameter settings of the Micro-plate reader. Please read the instructions carefully and adjust the instrument prior to the experiment.
5. Even the same operator might get different results in two separate experiments. In order to get reproducible results, the operation of every step in the assay should be controlled.
6. Every kit has strictly passed QC test. However, results from end users might be inconsistent with our data due to some variables such as transportation conditions, different lab equipment, and so on. Intra-assay variance among kits from different batches might arise from the above reasons, too.
7. Valid period: 6 months.